


BioPro CATHETER
REVISION A

Parts List			
ITEM	MATERIAL	PART NUMBER	DESCRIPTION
1	POLYVINYL CHLORIDE (PVC) PLASTIC	B1014	BioFlo DOMED TIP
2	POLYVINYL CHLORIDE (PVC) PLASTIC	B1004	BioFlo CANNULA TUBE
3	POLYVINYL CHLORIDE (PVC) PLASTIC	B1006	HANDLE

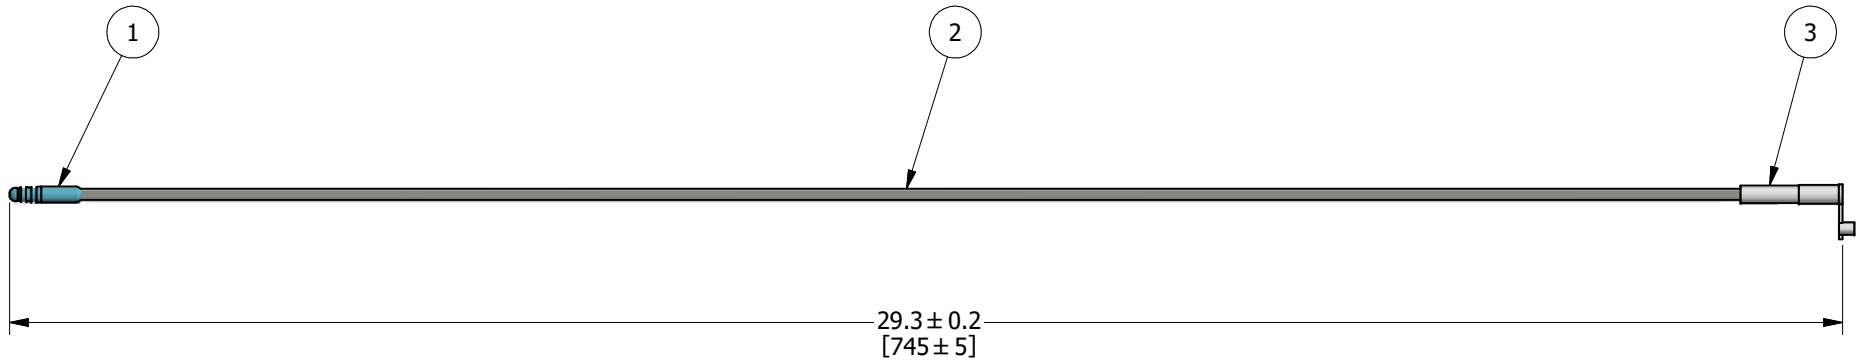

NOTES:

1. ALL MATERIALS USED ARE VIRGIN AND NON TOXIC RAW MATERIALS.
2. (ITEM 1), TIP IS ULTRASONICALLY WELDED TO THE CANNULA TUBE.
3. (ITEM 3), HANDLE IS GLUED TO CANNULA TUBE.
4. (ITEM 1), HAS A HINGED DOME.
5. SEE DRAWING B1017 FOR FURTHER ASSEMBLY DETAILS.
6. PACKED IN BAGS OF 10.
7. CASE CONTENTS ARE 5 LAYERS OF 100 CATHETERS FOR A TOTAL CASE COUNT OF 500 CATHETERS..
8. RIGID CARDBOARD TO SUPPORT EACH LAYER, APPROXIMATELY 4.8 MM THICK.

CHANGE RECORD		UNLESS OTHERWISE SPECIFIED:		Unless this drawing is being viewed from the file server of Ametek Switch, it is an UNCONTROLLED DOCUMENT. DESTROY ALL COPIES AFTER INITIAL USE!			
E.C. No.	DATE	DIMENSIONS ARE IN INCHES (MILLIMETERS):		FINISH CODE PER			
A. RLG	05-06-2020	TOLERANCES BELOW APPLY EXCEPT FOR VENDOR DESIGNED PARTS AND ITEMS PRODUCED TO RECOGNIZED STANDARDS.		ACTIVITY	REPLACED BY	REPLACES	
		PLOT DATE	FILE NAME	TITLE			
		---	SPEC SHEET	CannulaPro Catheter			
		FRACT. INCH ±	ANGLES ± 0.5°	DESCRIPTIVE DATA			
		DECIMAL-INCH	METRIC	DESIGNED	DRAWN	DATE	SCALE
		.0 ± .06	0. ± 1.5	MEA	RLG	04-15-2020	NONE
		.00 ± .03	0.0 ± 0.8	CHECKED	APPROVED	RECORDS	SHEET
		.000 ± .010	0.00 ± 0.25			04-15-2020	1 of 1
DO NOT SCALE DRAWING							
CONFIDENTIAL: This drawing, including all information contained therein, is the exclusive and confidential property of COMMON SENSE INSEMINATION PRODUCTS CO., of Las Vegas, NV 89121. This drawing is not to be copied, reproduced, delivered or disclosed to others, in whole or in part, except with express written permission.				CSIPCO LAS VEGAS, NEVADA 89121, U.S.A.		SIZE DWG. NO. SPEC SHEET	